

BeneHeart C2

SI & F -A I AED(A I E D)

SI & F



SI & E

SI & E




[Empty dashed orange text boxes for skilled responder instructions]




Unskilled

Remove pads package from lid of AED. Tear open package.
firmly
bare
.....

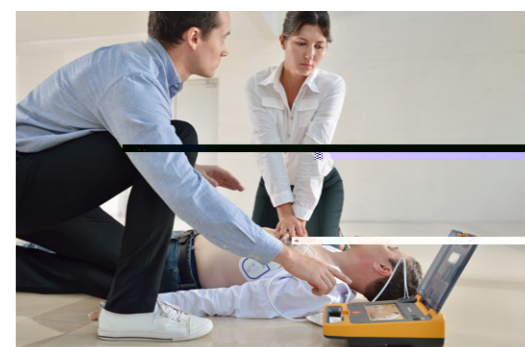




R, &D, Q,

1. 
[Empty box for notes]


2. 
[Empty box for notes]

3. 
[Empty box for notes]

4.
[Empty box for notes]

S C, S C

1.
[Empty box for notes]

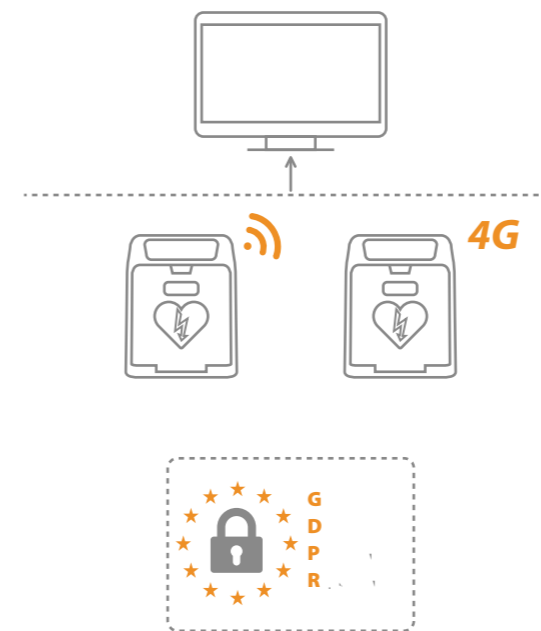

1.
[Empty box for notes]