


Passport[®] 8

Passport[®] 12

Quick Reference Guide

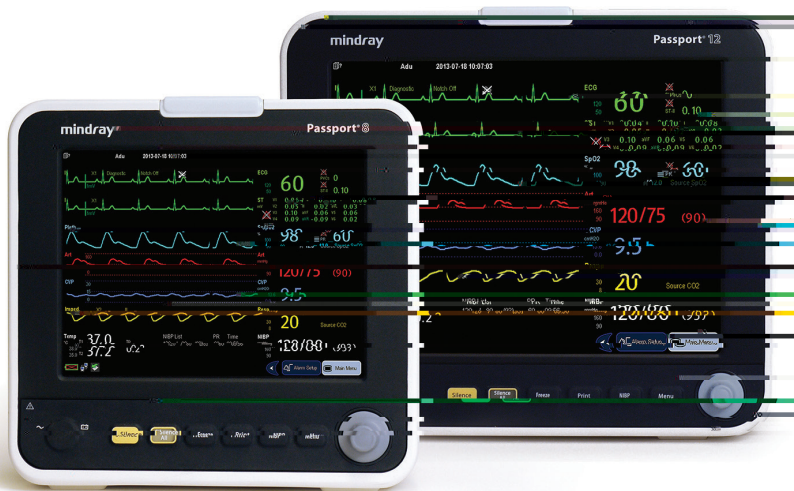

Note: The Passport 8 and Passport 12 Quick Reference Guide is not intended as a replacement to the Operating Instructions. Prior to operating equipment, the user must be familiar with the Operating Instructions Manual contents. This document is a guideline only to be used as an aid to comprehensive Inservice Training.

Table of Contents

Patient Setup	1
Admit Patient And Enter Demographics (Manual Entry)	1
Enter Demographics (Hospital Information System Interface)*	2
Adjust Patient Size	2
Discharge A Patient	3
Standb	4
Enter Standby	4
Record	4
Real-Time Waveforms	4
Adjust Recorder's Waveforms	5
Print	5
Real-Time Waveforms	5
ECG	5
Adjust Ecg Lead	5
Enable Pacemaker Detection And Set Pacemaker Rate	6
Initiate Relearn (Arrhythmia Option Required)	7
Initiate ST Analysis (ST Option Required)	7
NIBP	7
Initiate A Non-Invasive Blood Pressure Measurement (NIBP)	7
Set A Non-Invasive Blood Pressure Measurement Interval	8
Invasive Blood Pressures (Optional)	9
Adjust Invasive Blood Pressure Label	9
Zero Invasive Blood Pressure	9
Alarms	10
Adjust Alarm Limits	10
Adjust Alarm Responses	11
Adjust Arrhythmia Alarms (Arrhythmia Option Required)	12
Disable Non-Lethal Arrhythmia Alarms (Arrhythmia Option Required) ..	13

Table of Contents (cont'd)

Reset Alarms	13
Silence All Alarms	14
Transfer*	14
Hemodynamic Monitoring	15
Initiate A Cardiac Output Measurement	15
Initiate Pulmonary Artery Wedge Pressure (PAWP)	16
Initiate Hemodynamic Calculations	17
Screen Displa	18
Histor	20
Tabular Trends	20
Arrhythmia And Alarm Events	20
Full Disclosure	21
Volumes	22
Key Volume	22
Beat Tone	23
Alternate Operating Modes	23
Night Mode	23
Privacy Mode	24
Date And Time	25
Parameter Colors	26
Load Default (Preset) Settings	26
Lock/Unlocking Touchscreen Displa	27
Cleaning/Disinfecting	28
Cleaning the Main Unit/Module	28
Disinfecting the Main Unit/Module	30
Cleaning and Disinfecting the Accessories	31
Sterili ation	31

Display more QuickKeys

Hide the QuickKeys

Enter the main menu

PATIENT SETUP

Admit Patient And Enter Demographics (Manual Entr)

The Patient Setup menu allows the clinician to admit a patient and enter patient demographics. Admitting also restores default (preconfigured) settings and clears previous patient's information.



To admit a patient and enter demographics on the Passport 8 or Passport 12 bedside monitor:

- a. Select **Patient Setup** using **Pat** (or **1**) or **Main Menu** (or **2**)
 1. Select patient demographic field (Last Name, First Name, etc.)
 2. Enter patient's information using onscreen keyboard
 3. Select Yes or OK to enter Patient Demographics

Enter Demographics (Hospital Information System Interface)*

The Patient Setup menu allows the clinician to enter patient demographics from the Hospital Information System.

To enter demographics from the Hospital Information System on the Passport 8 or Passport 12 bedside monitor:

- a. Select **Patient Setup**>> using **Patient Setup**  (quick key) or **Main Menu** 

- d. Select current size and adjust to Adu (adult), Ped (pediatric), or Neo (Neonate)
- e. Select **OK** to return to main display

Note: Adjusting patient size restores the monitor to the default (preconfigured) settings but does not clear patient information or data.



DPM Central Station: Patient size can be changed on the DPM Central Station.

Panorama Central Station: Patient size cannot be changed on the Panorama Central Station.

Discharge A Patient

The Discharge function clears all patient information and restores default (preconfigured) settings.

To Discharge a patient on the Passport 8 or Passport 12 bedside monitor:


- a. Select **Patient Setup**>> using **Patient Setup**  (quick key) or **Main Menu** 

STANDBY

Enter Standb

The Standby function allows the clinician to suspend monitoring on a patient. While in standby, the patient is not monitored; however, all data and settings are preserved.

To place a patient into Standby on the Passport 8 or Passport 12 bedside monitor:

Select the **STANDBY**  (quick key) and select **Yes** to confirm. To remove a patient from Standby and resume monitoring on the Passport 8 or Passport 12 bedside monitor select any key on the Passport 8 or Passport 12 bedside monitor.

DPM Central Station Interface: Selecting **Standb** on the Passport 8 or Passport 12 bedside monitor automatically places the DPM Central Station in standby. Select any key on the Passport 8 or Passport 12 bedside monitor to remove patient from Standby. Selecting **Standb** in the patient's drop down menu will remove patient from standby.

Panorama Central Station Interface: Selecting **Standb** on the Passport 8 or Passport 12 bedside monitor automatically places the Panorama Central Station, WorkStation, and ViewStation in standby. Selecting **Bedside and Panorama Standb** on the Panorama Central Station or WorkStation automatically places the bedside monitor and ViewStation in standby. Select any key on the Passport 8 or Passport 12 bedside monitor to remove patient from Standby as a patient cannot be removed from Standby on the Panorama Central Station.



RECORD

Real-Time Waveforms

To record a strip on a patient on the Passport 8 or Passport 12 bedside monitors' integrated recorder select **Record** on the monitor's front key pad.


Adjust Recorder's Waveforms

To adjust recorded waveforms on a patient on the Passport 8 or Passport 12 bedside monitors' integrated recorder:

- a. **Main Menu**  (quick key)
- b. Select **Record Setup** >>
- c. Select **Waveform 1, Waveform 2, or Waveform 3**
- d. Select the waveforms for recording from drop down list or select off to turn off waveform recording
- e. Select **Main Menu**  (quick key) or **X** to return to the main display

PRINT

Real-Time Waveforms

To print a strip on a patient on the Passport 8 or Passport 12 bedside monitor to a predetermined laser printer select **Real-Time Print**  (quick key).

DPM Central Station Interface: Selecting **Real-Time Print** on the Passport 8 or Passport 12 bedside monitor will print a 10-second, Real-Time Report on the DPM Central Station. The waveforms printed are determined by the Passport 8 or Passport 12 bedside monitor.

Panorama Central Station Interface: Selecting **Real-Time Print** on the Passport 8 or Passport 12 bedside monitor will print a 10-second, All Strips Report on the Panorama Central Station. The waveforms printed are determined by the **Print Setup** tab on the Panorama Central Station. Waveform print selection on the Panorama Central Station, WorkStation, and ViewStation are independent

ECG



Adjust ECG Lead

The Passport 8 or Passport 12 bedside monitor allows the clinician to adjust the leads being viewed on the main display. To adjust the ECG Lead:

- a. Select ECG waveform or ECG numeric tile to enter the **ECG Setup** menu





Or

- a. Select **ECG Setup>>** by selecting ECG waveform/ HR numeric tile or from **Parameters** menu  or **Main Menu** 

Panorama Central Station Interface: Pacemaker detection on the Passport 8 or Passport 12 bedside monitor, Panorama Central Station, WorkStation, and ViewStation are independent.

Initiate Relearn (Arrhythmia Option Required)

To initiate relearning manually on the Passport 8 or Passport 12 bedside monitor:

- a. Select **ECG Setup >>** by selecting ECG waveform/HR numeric tile or from **Parameters** menu () or **Main Menu** ()

DPM Central Station Interface: Selecting **Start NIBP Measurement** on the DPM Central Station will initiate a NIBP measurement on the Passport 8 or Passport 12 bedside monitor.



Set A Non-Invasive Blood Pressure Measurement Interval

The Passport 8 or Passport 12 bedside monitor allows the clinician to set an interval for a NIBP measurement to be obtained automatically.

To set an automatic interval on the Passport 8 or Passport 12 bedside monitor:

- a. Select NIBP measurement  (quick key) and Select interval

Or


- a. Select **NIBP >>** by selecting NIBP tile or from **Parameters** menu ()
or **Main Menu** 

INVASIVE BLOOD PRESSURES (OPTIONAL)

The Passport 8 allows a clinician to monitor up to 2 invasive blood pressures (IBP) with the included Y-type IBP adapter and external module. The Passport 12 bedside monitors allow a clinician to monitor up to 4 invasive blood pressures (IBP) simultaneously with 2 invasive blood pressure (IBP) ports on the Passport 12 and 2 additional invasive blood pressure (IBP) with the included Y-type IBP adapter and external module.

Adjust Invasive Blood Pressure Label

To adjust the label on an invasive blood pressure on the Passport 8 or Passport 12 bedside monitor:


- a. Insert IBP Module as needed
- b. Select the Invasive Blood Pressure (ART, CVP, etc.) Setup >> by selecting IBP waveform/tile or from Parameters menu ( or Main Menu

ALARMS

Adjust Alarm Limits

The Alarm Setup tab allows the clinician to configure alarm limits and alarm responses on the Passport 8 or Passport 12 bedside monitors.

To adjust a patient's alarm limit on the Passport 8 or Passport 12 bedside monitor:


- a. Select parameter's waveform or numeric tile to open parameters Setup menu
- b. Select **Alarm Setup >>**
- c. Select High or Low limit value and adjust using the up and down arrows
- d. Select Off in the limit value area to disable the parameter's alarm limit(s)
- e. Select **Main Menu**  (quick key) or **X** to return to the main display

Or

- a. Select **Alarm Setup>>** from

Adjust Alarm Responses

To adjust a patient's alarm responses on the Passport 8 or Passport 12 bedside monitor:

- a. Select parameter's waveform or numeric tile to open parameters Setup menu
- b. Select **Alarm Setup >>**
- c. Select
 - **On/Off** – Enable/disable the alarm's responses
 - **Level** – to adjust the audio and visual alarm indicators. Level options include High (Red), Medium (Yellow), and Low (Yellow)*
 - **Record** – to activate an automatic recording when the alarm occurs
 - **Print (DPM Central Station Interface)** prints patient's alarm settings to designated laser printer
 - **Default** – to restore preset settings
- d. Select **Main Menu**  (quick key) or **X** to return to the main display

Or




- a. Select **Alarm Setup >>** from  (quick key) or **Main Menu**  (quick key)

DPM Central Station Interface: Changing alarm responses on the DPM Central Station will not change alarm responses on the Passport 8 or Passport 12 bedside monitor. Changing alarm responses on the Passport 8 or Passport 12 bedside monitor will not change alarm responses on the DPM Central Station.

Panorama Central Station Interface: Changing alarm responses the Panorama Central Station or WorkStation will not change alarm responses on the Passport 8 or Passport 12 bedside monitor. Changing alarm responses on the Passport 8 or Passport 12 bedside monitor will not change alarm responses on the Panorama Central Station and WorkStation.

Adjust Arrhythmia Alarms (Arrhythmia Option Required)

To adjust a patient's arrhythmia alarm on the Passport 8 or Passport 12 bedside monitor:

- a. Select **Alarm Setup** >> from  (quick key) or **Main Menu**  (quick key)
- b. Select **Arrh. Analysis** tab
- c. Scroll and select individual arrhythmia
- d. Select
 - **Alarm** – to enable or disable arrhythmia alarm notification
 - **Alm Lev** – to adjust the audio and visual alarm indicators. Level options include High (Red), Medium (Yellow), and Low (Yellow) and Message* (audio absent)
 - **Alm Rec** – to activate an automatic recording when the alarm occurs
- e. Select **Main Menu**  (quick key) or **X** to return to the main display

*Arrhythmia dependent




DPM Central Station Interface: Adjusting arrhythmia alarms on the DPM Central Station or WorkStation will not change arrhythmia alarms on the Passport 8 or Passport 12 bedside monitor. Adjusting arrhythmia alarms on the Passport 8 or Passport 12 bedside monitor will affect the arrhythmia alarm on the DPM Central Station.

Panorama Central Station Interface: Adjusting arrhythmia alarms on the Panorama Central Station or WorkStation will not change arrhythmia alarms

on the Passport 8 or Passport 12 bedside monitor. Adjusting arrhythmia alarms on the Passport 8 or Passport 12 bedside monitor will affect the arrhythmia alarm on the Panorama Central Station and WorkStation.


Disable Non-Lethal Arrhythmia Alarms (Arrhythmia Option Required)

To disable all arrhythmia alarms *except lethal* arrhythmias on the Passport 8 or Passport 12 bedside monitor:

- a. Select **Alarm Setup >>** from  (quick key) or **Main Menu**  (quick key)
- b. Select **Arrh. Analysis** tab
- c. Select **Lethals On**
- d. Select **Main Menu**  (quick key) or

Station, WorkStation, and ViewStation for a *preconfigured amount of time*. Selecting **Mute** on the Panorama Central Station *will not* silence an alarm on the Passport 8 or Passport 12 bedside monitor.

SILENCE ALL ALARMS

To silence *all alarms* on the Passport 8 or Passport 12 bedside monitor for a preconfigured amount of time, select **Alarm Pause**  key on front panel of bedside monitor.



DMP Central Station Interface: Selecting **Alarm Pause** on the Passport 8 or Passport 12 bedside monitor will silence active alarms on the Panorama Central Station, WorkStation, and ViewStation for a *preconfigured amount of time*. Selecting **Alarm Pause** on the Panorama Central Station will silence alarms on the Passport 8 or Passport 12 bedside monitor.

Panorama Central Station Interface: Selecting **Alarm Pause** on the Passport 8 or Passport 12 bedside monitor will silence active alarms on the Panorama Central Station, WorkStation, and ViewStation for a *preconfigured amount of time*. Selecting **Mute** on the Panorama Central Station *will not* silence alarms on the Passport 8 or Passport 12 bedside monitor.

TRANSFER*

The Passport 8 or Passport 12 bedside monitors have the ability to transfer patient data through a storage medium (USB Flash Drive)

To transfer patient data from one Passport 8 or Passport 12 bedside monitor to another Passport 8 or Passport 12 bedside monitor:

- a. Insert USB Flash Drive into USB port on back of monitor
- b. Select **Patient Setup** >> using **Patient Setup**  (quick key) or **Main Menu**  (quick key)
- c. **Select Transfer to Storage Medium***
- d. Select **OK**
- e. Remove USB Flash Drive once **Transfer to storage medium successful** message is displayed
- f. Insert USB Flash Drive into USB port on back of new Passport 8 or Passport 12 bedside monitor

g. Select **Transfer**

1. Select Trends to transfer patient's trended data (configurable)
2. Select Alarm Events to transfer patient's alarm events
3. Select Alarm Limits to transfer patient's alarm settings

h. Select **Yes** to confirm

i. Confirm **Transfer from storage medium successful** message is displayed

j. Select to unload (release USB Flash Drive) and select **OK**

k. Remove USB Flash Drive

*If enabled

DPM Central Station Interface: Transferring patient data from one Passport 8 or Passport 12 bedside monitor to another Passport 8 or Passport 12 bedside monitor will not transfer data within the DPM Central Station. Transferring data within a DPM Central Station or to a different DPM Central Station may affect the Passport 8 or Passport 12 bedside monitor.


Panorama Central Station Interface: Transferring patient data from one Passport 8 or Passport 12 bedside monitor to another Passport 8 or Passport 12 bedside monitor will not transfer data within the Panorama Central Station. Transferring data within a Panorama Central Station or to a different Panorama Central Station may affect the Passport 8 or Passport 12 bedside monitor.

HEMODYNAMIC MONITORING



Initiate A Cardiac Output Measurement

Cardiac Output (C.O.) is the amount of blood ejected from the left ventricle each minute, expressed in liters per minute (l/min). Cardiac Index (CI) is the Cardiac Output divided by the patient's body surface area.

To initiate a Cardiac Output measurement on the Passport 8 or Passport 12 bedside monitor:

- a. Insert IBP/C.O. Module
- b. Connect the C.O. cable to the C.O. connector on the monitor interconnecting the C.O. Module, PA Catheter, and injectate.
- c. Select **C.O. Setup >>** by selecting C.O. tile,  (quick key), or from

Parameters >> ( or Main Menu 

- i. Select
 1. **Cancel** to stop the current measurement
 2. **Record** to record the most recent cardiac output measurement and numeric data
- j. Select **Main Menu**  (quick key) or  to return to the main display

Or

- j. Select **Calc>>** to access the Hemodynamic Calculations menu



Note: Blood temperature alarms are inactive when a cardiac output measurement is initiated.

Initiate Pulmonar Arter Wedge Pressure (PAWP)

Pulmonary Artery Wedge Pressure (PAWP) is a pressure measurement derived from a PA catheter when the PA distal balloon is inflated and the catheter advances and occludes a distal pulmonary artery. PAWP pressure is a reflection of the pressure in the left ventricle at end-diastole.

To initiate a PAWP measurement on the Passport 8 or Passport 12 bedside

automatically entered from the current values along with height and weight if previously entered

- c. Select remaining parameter and manually enter
- d. Select **Calculate** to complete calculation
- e. Select **Record** to print the currently displayed Hemodynamic Calculations
- f. **Main Menu**  (quick key) or  to return to the main display (quick key) on main o

- **O CRG Screen:** Split screen with oxyCRG (HR trend, SPO₂ trend, and RR trend/RR waveform) on the lower portion of the display with real time waveforms and numeric parameters
- **View Others Screen (optional):** Split screen with viewing information from another bed(s) on the lower portion of the display with real time waveforms and numeric parameters on the host monitoring device
- **ECG 7-Lead Half-Screen:** (5 lead wire set): 7 Leads of ECG on the upper portion with real time waveforms and numeric parameters on the main display
- **ECG 7-Lead Full Screen:** (5 lead wire set): 7 leads of ECG with numeric parameters on the main display
- **ECG 12-Lead Full Screen (Optional):** 12 leads of ECG with numeric parameters on the main display (for Passport 12 bedside monitor only)
- **PAWP Screen (Optional):** Split screen with PAWP measurement window on the lower portion of the main display with real time waveforms and numeric parameters
- **C.O. Screen (Optional):** Split screen with C.O. measurement window on the upper portion of the main display with real time waveforms and numeric parameters

Note: The first waveform is always an ECG lead and HR is always located in the first digital tile in the Normal Screen selection.

DPM Central Station Interface: Digital and waveform display selections on the DPM Central Station are independent of the Passport 8 or Passport 12 bedside monitor.

Panorama Central Station Interface: Digital and waveform display selections on the Panorama Central Station, WorkStation, and ViewStation are independent of the Passport 8 or Passport 12 bedside monitor.

HISTORY



Tabular Trends





To display Tabular (List) trends on a patient on the Passport 8 or Passport 12 bedside monitor:

- a. Select **Revie** >>  (quick key) or from **Main Menu** 

To view and print an alarm event on a patient on the Passport 8 or Passport 12 bedside monitor:

- a. Select **Review** >>  (quick key) or from **Main Menu**  (quick key)

To record waveforms stored on a patient:

- a. Select **Revie** >>  (quick key) or from **Main Menu**  (quick key)
Select **Full Disclosure** tab
- b. Select **Record** to record the first three saved waveforms



DPM Central Station Interface: Waveform Review (Disclosure) storage and printing on the Passport 8 or Passport 12 bedside monitor and DPM Central Station are independent.

Panorama Central Station Interface: Full disclosure storage and printing on the Passport 8 or Passport 12 bedside monitor and Panorama Central Station are independent.

VOLUMES

The alarm volume, key volume, and QRS volume can be adjusted on the Passport 8 or Passport 12 bedside monitors.



To adjust the alarm volume on the Passport 8 or Passport 12 bedside monitor:

- a. Select **Volume**  (quick key) or select **Others** Tab in **Alarm Setup** (quick key)
- b. Select **Alm Vol**
- c. Select volume ranging from X*-10 (0=Off 10=Max)
- d. Select **Main Menu**  (quick key) or **X** to return to the main display

* The minimum volume range (X) is predetermined during installation.


Ke Volume

To adjust the key volume on the Passport 8 or Passport 12 bedside monitor:


- a. Select **Volume**  (quick key)
- b. Select **Ke Vol**
- c. Select volume ranging from 0-10 (0=Off 10=Max)
- d. Select **Main Menu** 

Beat Tone

To adjust the beat tone (QRS tone) volume on the Passport 8 or Passport 12 bedside monitor:

- a. Select ECG waveform or ECG numeric tile to enter **ECG Setup>>**
- b. Select **Others>>**
- c. Select **QRS Volume**
- d. Select volume ranging from 0-10 (0=Off 10=Max)
- e. Select **Main Menu**  (quick key) or **X** to return to the main display

Or

- a. Select SPO₂ waveform or SPO₂ numeric tile to enter **SPO₂ Setup>>**
- b. Select **Beat Vol**
- c. Select volume ranging from 0-10 (0=Off 10=Max)
- d. Select **Main Menu** 

b. Select **Enter Night Mode**

To remove a patient from Night Mode:

- a. Select **Night Mode**  (quick key)

Or

- a. Select **Main Menu** 

DATE AND TIME

To adjust the date and time on the Passport 8 or Passport 12 bedside monitor:

- a. Select **Date/Time** next to patient size on main display
- b. Set the date and time
- c. Select **Date Format** to adjust the month, day, and year format
- d. Select **Time Format** to adjust the time format (12h or 24h)

Or





- a. Select **Main Menu** 

Adjusting the date and time on the

PARAMETER COLORS

The Passport 8 or Passport 12 bedside monitor provides the ability to adjust the parameter's numeric and waveform (if applicable) color.

To adjust the parameter's color on the Passport 8 or Passport 12 bedside monitor:

- a. Select **Main Menu**  (quick key)
- b. Select **Screen Setup**>>
- c. Select **Measurement Color Setup** >>
- d. Select parameter 
- e. Select color 
- f. Select **Main Menu**  (quick key) or **X** to return to the main display


DPM Central Station Interface: Parameter color on the Passport 8 or Passport 12 bedside monitor and DPM Central Station are independent.

Panorama Central Station Interface: Parameter color on the Passport 8 or Passport 12 bedside monitor, Panorama Central Station, ViewStation, and WorkStation are independent.

LOAD DEFAULT (PRESET) SETTINGS

The Passport 8 or Passport 12 bedside monitors settings are automatically restored either when the patient size is adjusted or when Discharge is performed.

A clinician may restore default settings on patient currently being monitored on the Passport 8 or Passport 12 bedside monitor by:

- a. Select **Main Menu** 

LOCK/UNLOCKING TOUCHSCREEN DISPLAY

The Passport 8 or Passport 12 bedside monitor provides the ability to lock and unlock the touchscreen display.

To lock the touchscreen display on the Passport 8 or Passport 12 bedside monitor press and hold **Main Menu**  (quick key) for 2-3 seconds until



CLEANING/DISINFECTING



Cleaning the Main Unit/Module

Clean your equipment on a regular basis. Before cleaning, consult your hospital's regulations for cleaning the equipment.

The following table lists approved cleaning and disinfecting agents.

Product Name	Product Type	Ingredients
Sodium hypochlorite bleach*	Liquid	Sodium hypochlorite bleach 0.5%
Hydrogen peroxide*		Hydrogen peroxide 3%
Isopropanol*		Isopropanol 70%
1-Propanol*		1-Propanol 50%
CIDEX OPA Solution		Ortho-Phthalaldehyde 0.55%
Metrex CaviCide1™		Diisobutylphenoxyethoxyethyl dimethyl benzyl ammonium chloride 0.28%, Isopropanol 17.2%
Virex® II 256		Didecyl dimethyl ammonium chloride 8.704%, n-Alkydimethyl benzyl ammonium chloride 8.190%
Virex®TB		n-Alkyl dimethyl benzyl ammonium chlorides 0.105%, n-Alkyl dimethyl ethylbenzyl ammonium chlorides 0.105%
Rely+On™ Virkon®Powder *(Used as 1% solution)	Powder	Used as 1% solution Biocidal active: Pentapotassium bis (peroxymonosulphate) bis (sulphate)(500g/kg), Contains dipotassium peroxodisulphate.

Product Name	Product Type	Ingredients
PDI Sani-Cloth® Plus Germicidal Disposable Cloth	Wipes	n-Alkyl dimethyl ethylbenzyl ammonium chlorides 0.125%, n-Alky dimethyl benzyl ammonium chlorides 0.125%
PDI Super Sani-Cloth®Germicidal Disposable Wipe		n-Alkyl dimethyl ethylbenzyl ammonium chlorides 0.25%, n-Alkyl dimethyl benzyl ammonium chlorides 0.25%, Isopropyl Alcohol 55.0%,
VIRAGUARD Hospital Surface Disinfectants		Isopropanol 70%,Other ingredients 30%

Note: For equipment with the symbol , all the listed cleaning and disinfecting agents are available for use. For equipment without the symbol , only the cleaning and disinfecting agents marked with "*" are available for use.

To clean the equipment:

- a. Shut down the monitor and disconnect it from AC power.
- b. Clean the display screen with wipes or a soft cloth moistened with one of the cleaning agents listed in the table above.
- c. Clean the exterior surface of the equipment or module with wipes or a soft cloth moistened with one of the cleaning agents listed in the table above. Avoid wetting the pins and metal parts.
- d. Wipe off all the residue with a dry cloth.
- e. Dry your equipment in a ventilated, cool place.

Disinfecting the Main Unit/Module

Disinfect your equipment as required in your hospital's servicing schedule using one of the disinfecting agents listed in the table above. Cleaning equipment before disinfecting is recommended.

Cleaning and Disinfecting the Accessories

For information about cleaning and disinfecting of accessories, please refer to the manufacturer's packaging or the Passport 8/Passport 12 Patient Monitor Operator's Manual.

STERILIZATION

Sterilization is not recommended for this equipment, related products, accessories, or supplies unless otherwise indicated in the Instructions for Use that accompany the products, accessories or supplies.

Mindray DS USA, Inc.
800 MacArthur Blvd., Mahwah, NJ 07430
Tel: 800.288.2121 or 201.995.8000
www.mindray.com



046-005847-00(3.0)

mindray
NORTH AMERICA